




<Sample Information>

Sample Name : 1515-12 Additional vial tested TB-500, Black top
Sample ID :
Data Filename : 1515-12 Additional vial tested TB-500, Black top_TFA screening gradient 5-95%_159.
Method Filename : TFA screening gradient 5-95%.lcm
Batch Filename : 240313.lcb
Vial # : 1-53
Injection Volume : 0.5 uL
Date Acquired : 14.03.2024 1:55:02
Date Processed : 18.03.2024 13:35:36

Sample Type : Unknown
Acquired by : Janoshik s.r.o.
Processed by : Janoshik s.r.o.

<Chromatogram>

mAU

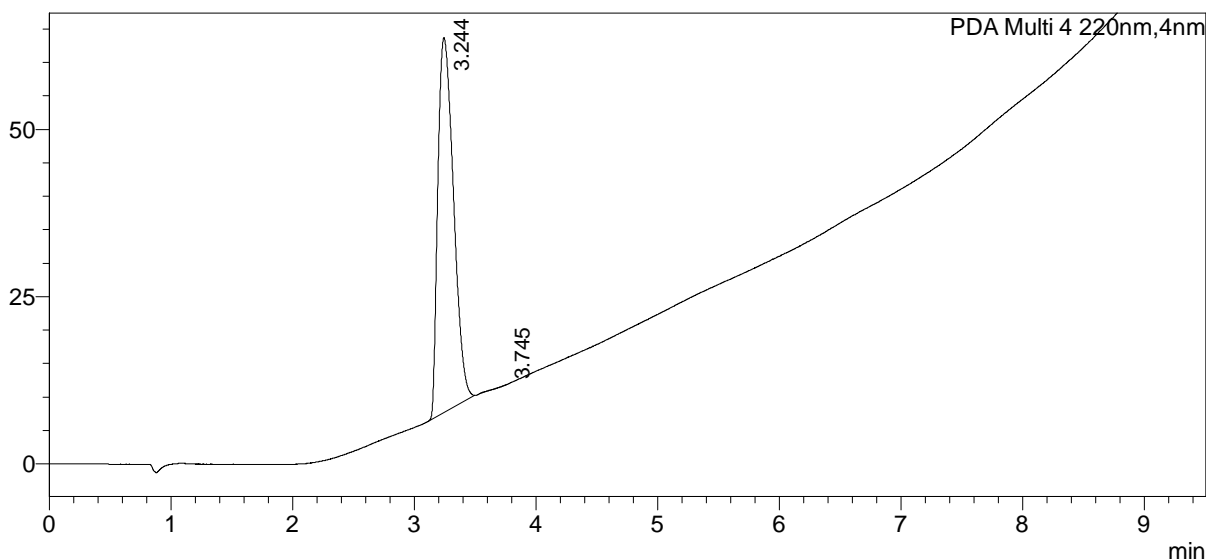

<Peak Table>

PDA Ch4 220nm

Peak#	Ret. Time	Area	Area%	Conc.	Unit	Name
1	3.244	502201	99.974	0.00		
2	3.745	131	0.026	0.00		
Total		502332	100.000			